

Fig. 1

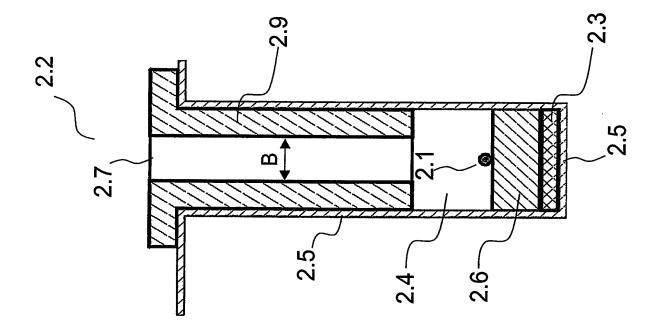


Fig. 2

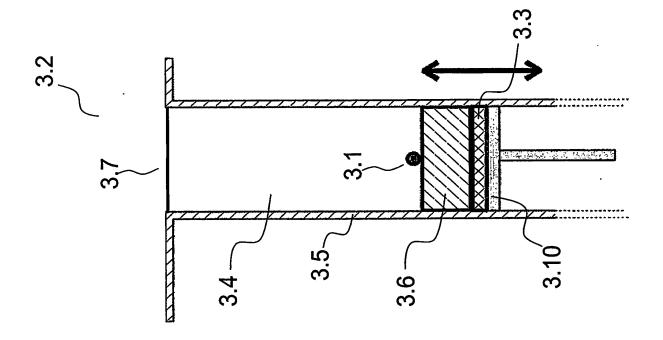


Fig. 3

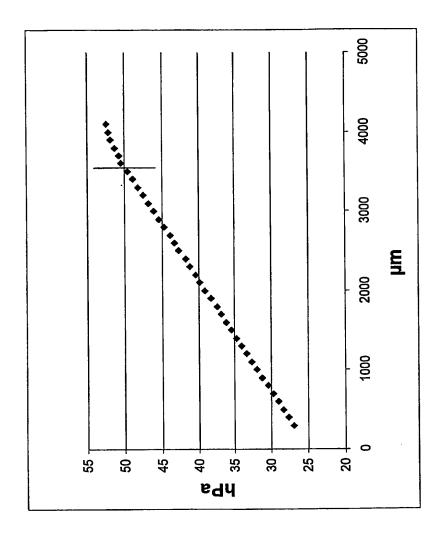


Fig. 4

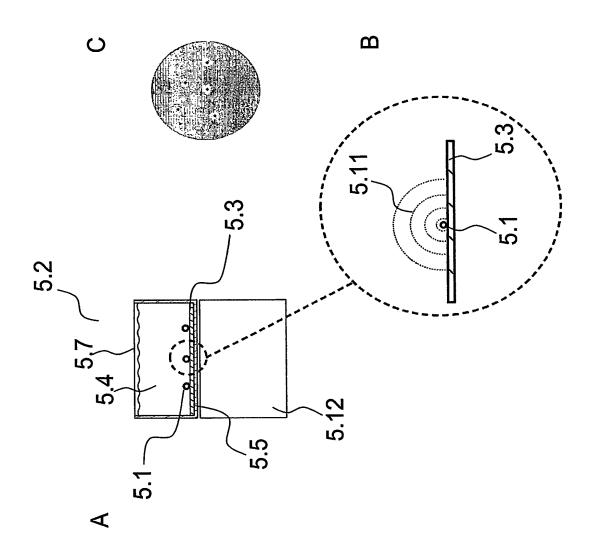
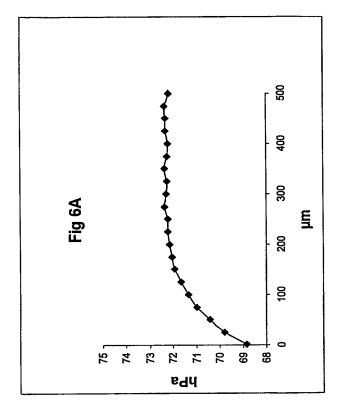


Fig. 5



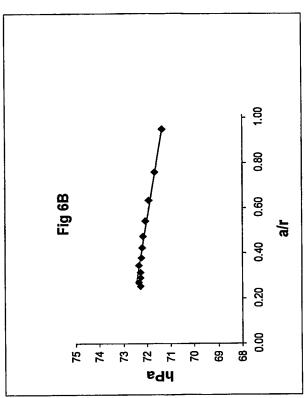


Fig. (6

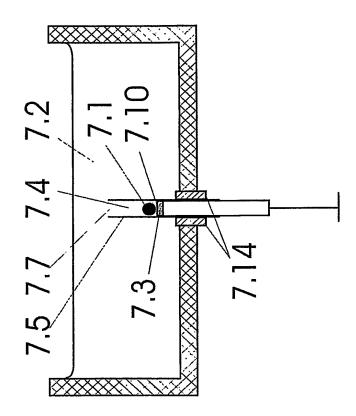


Fig. 7

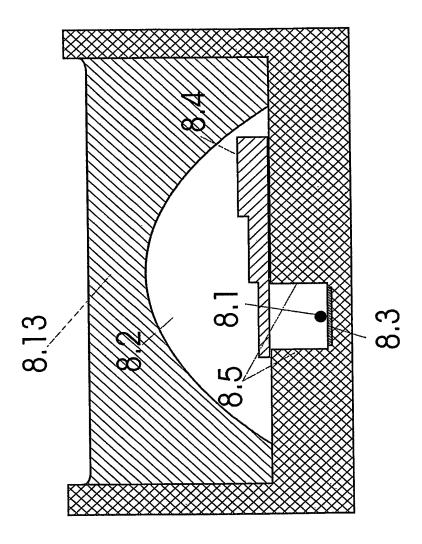


Fig. 8

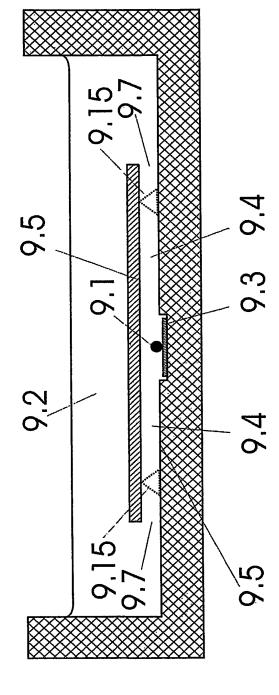
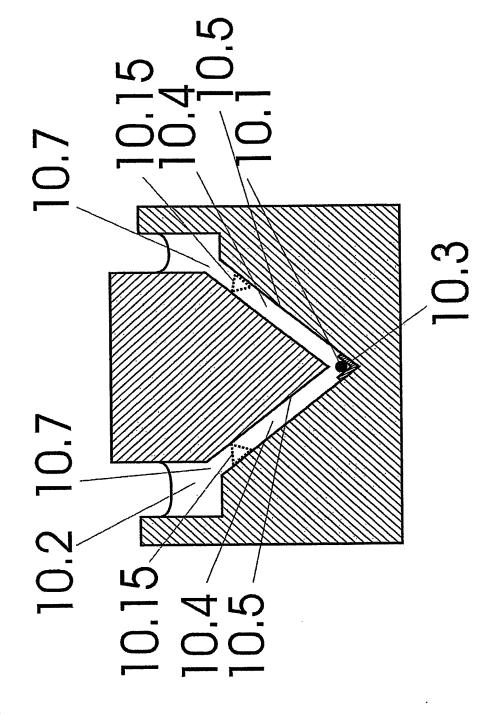


Fig. 9

Fig. 10



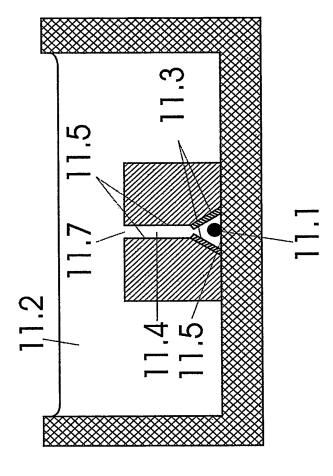


Fig. 1

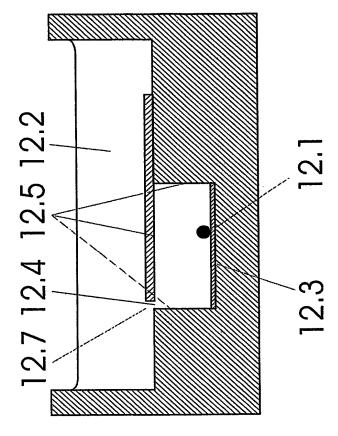


Fig. 12

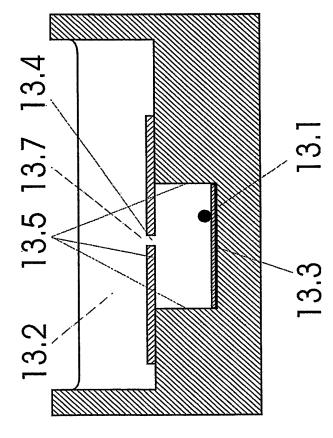
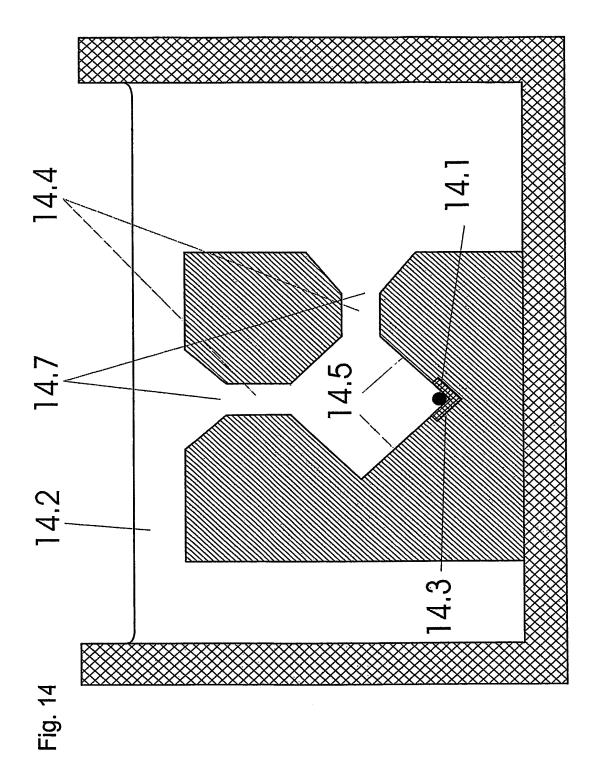


Fig. 13





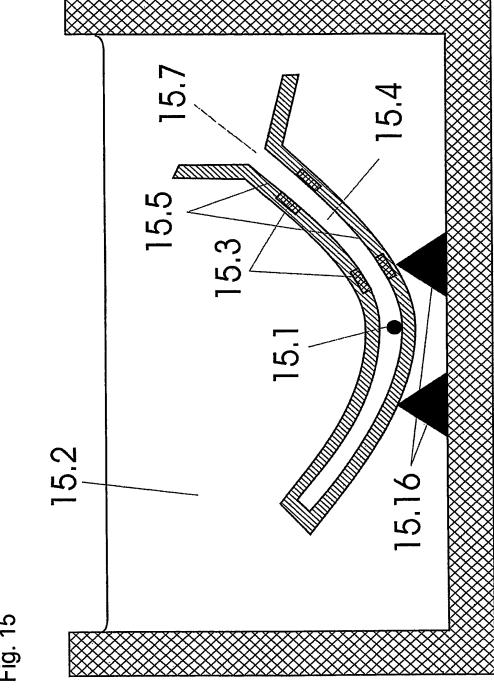


Fig. 1

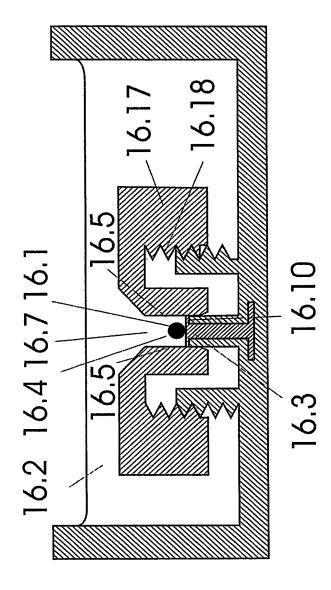

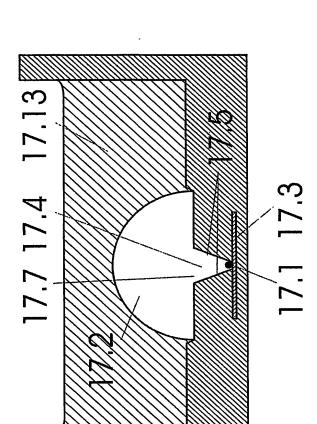

PCT/DK2003/000935

Fig. 17

Fig. 18



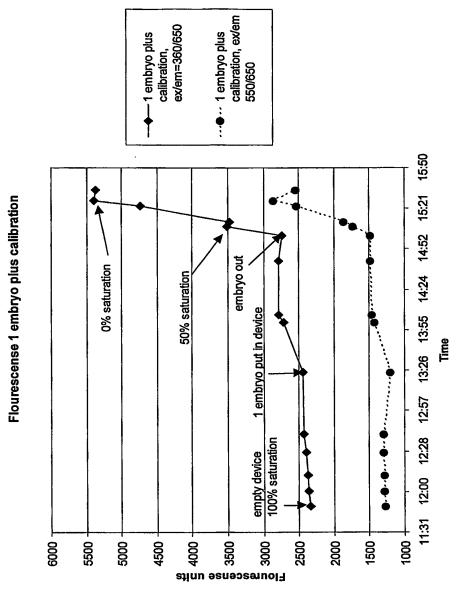


Fig. 19

Calibrated values,

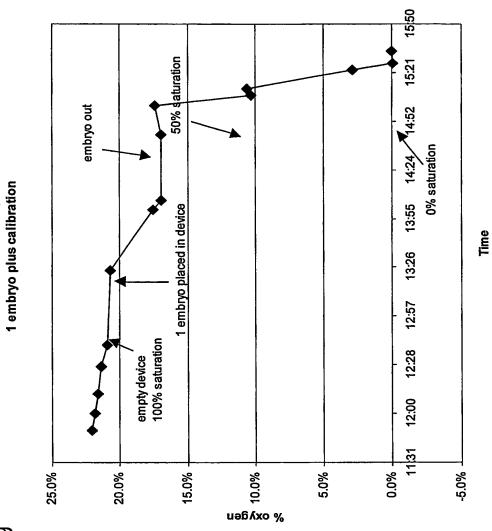

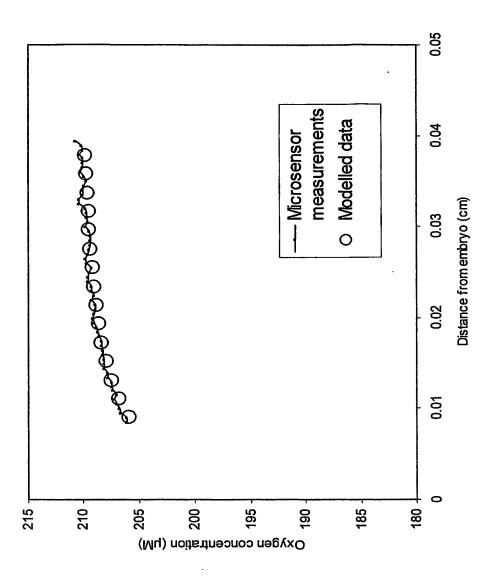

-ig. 20